

# Bifix® Hybrid Abutment Instructions



CONTENT:

page







<b>Laboratory</b>	<b>A</b>	<b>Try-In</b>	3
<hr/>			
	<b>B</b>	<b>Preparation</b>	
	B-I	metal, titanium	4
		or	
	B-II	silicate ceramic	5
		or	
	B-III	oxide ceramic / composite	6
<hr/>			
	<b>C</b>	<b>Application</b>	7
<hr/>			
<b>Dental practice</b>	<b>A</b>	<b>Try-In</b>	8
<hr/>			
	<b>B</b>	<b>Preparation</b>	
	B-I	metal, titanium	9
		or	
	B-II	silicate ceramic	10
		or	
	B-III	oxide ceramic / composite	11
<hr/>			
	<b>C</b>	<b>Application</b>	12



= Read manufacturer instructions before use





# Laboratory

## A Try-In

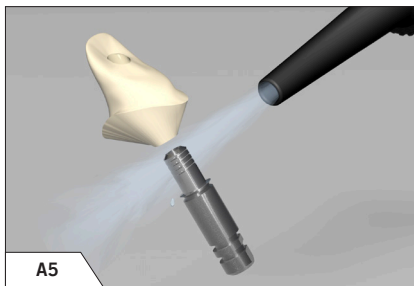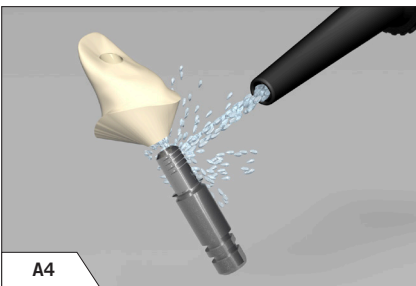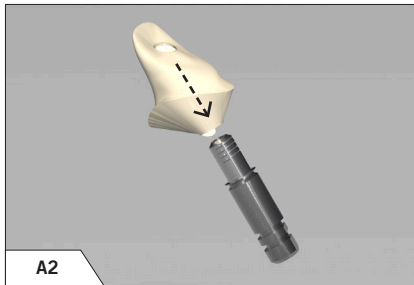



# Laboratory





<b>B</b>	<b>Preparation</b>	<b>B-I</b>	metal, titanium
----------	--------------------	------------	-----------------

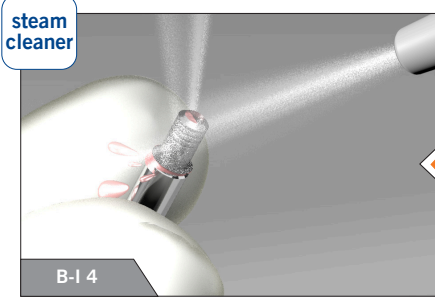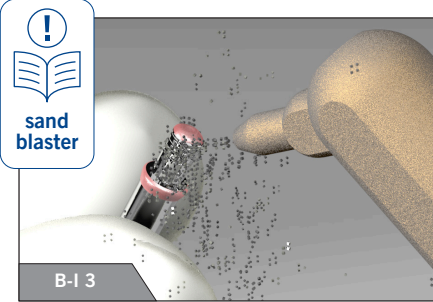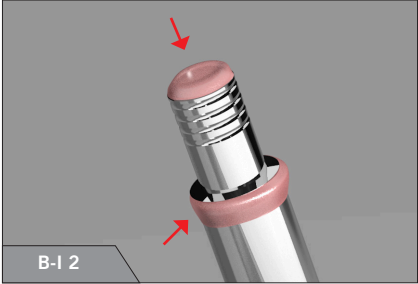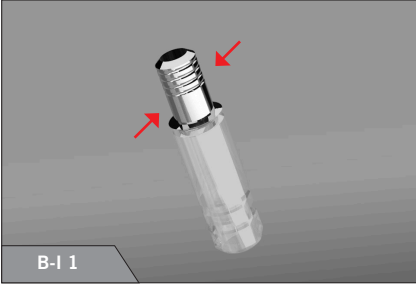

or








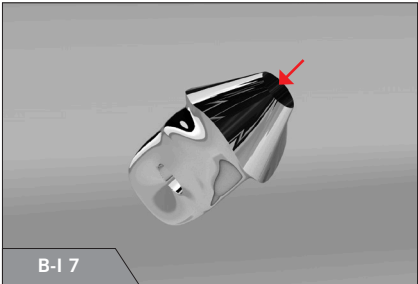


=

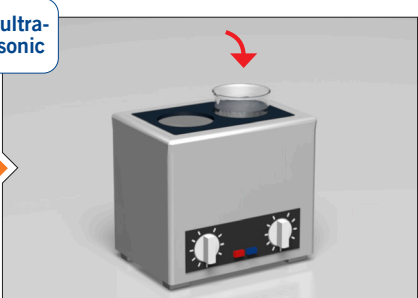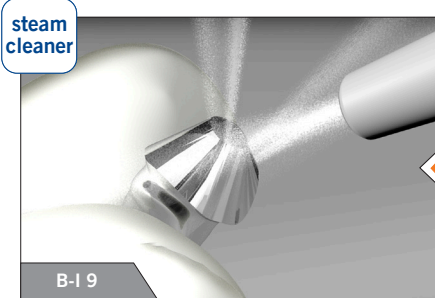






# Laboratory

<b>B</b>	<b>Preparation</b>	<b>B-II</b> silicate ceramic
----------	--------------------	------------------------------

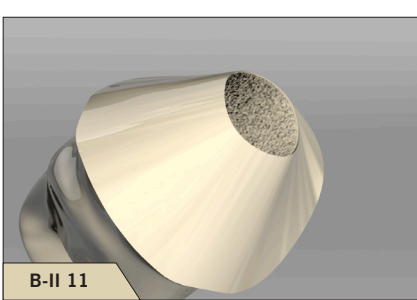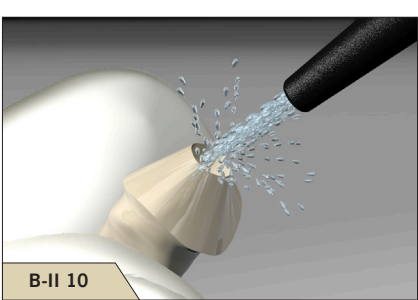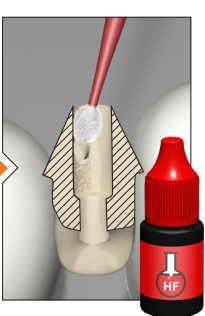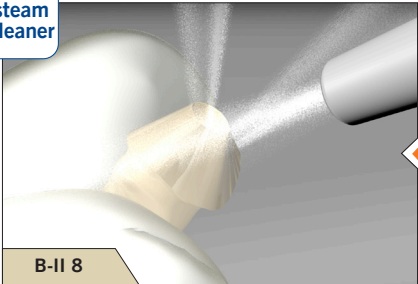
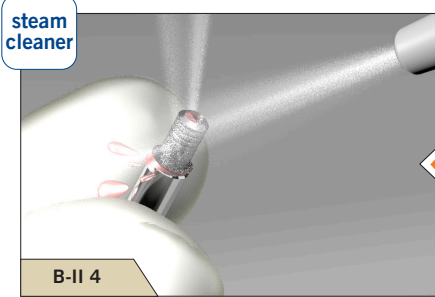
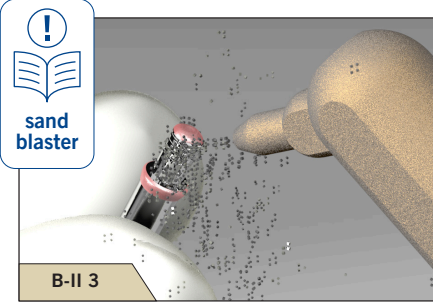
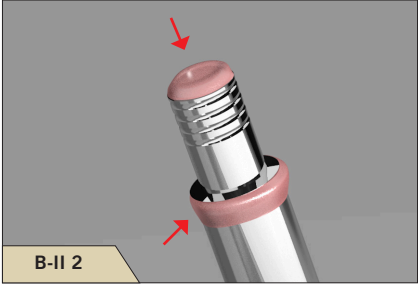
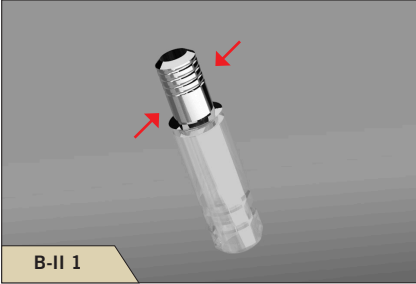


# Laboratory


<b>B</b>	<b>Preparation</b>	<b>B-III</b> oxide ceramic /composite
----------	--------------------	---------------------------------------

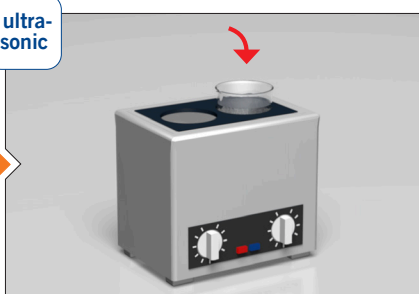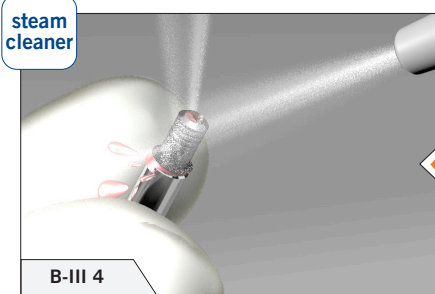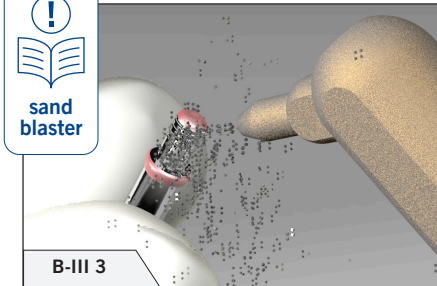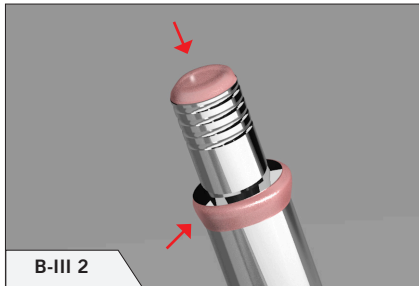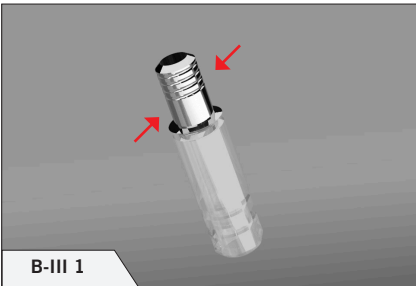

or

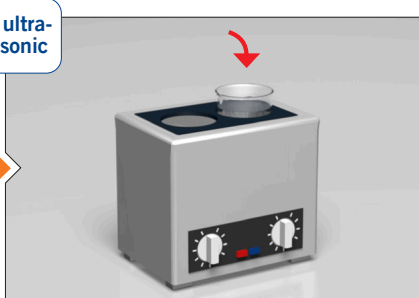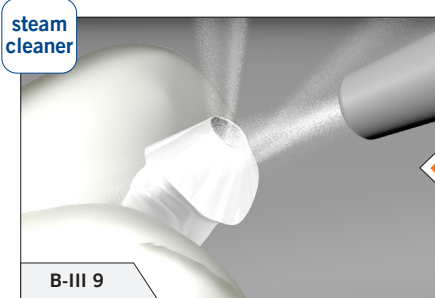

or

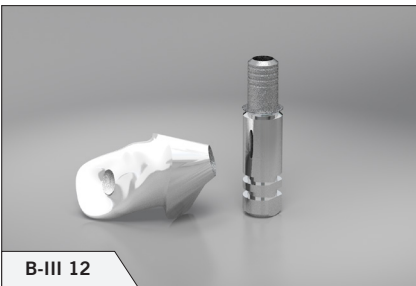

Laboratory



C Application

**C1** 60 sec.

**C2** 60 sec.

**C3**

**C4**

**C5**

**C6**

**C7**

**C8** Glycerine

**C9** ca. 7 min. PRESS

**C10**

**C11**

**C12**







Dental practice



A Try-In








Occlu  
Check

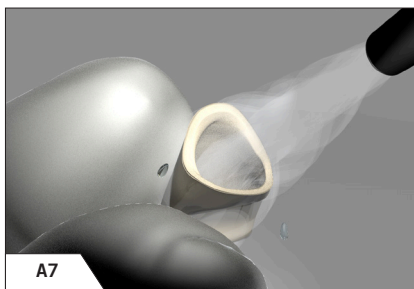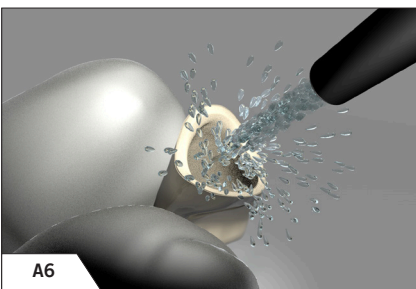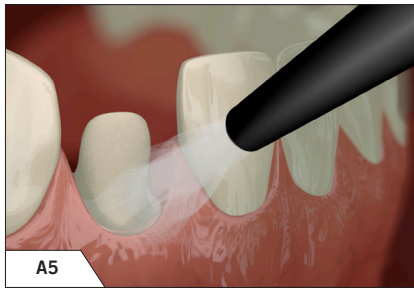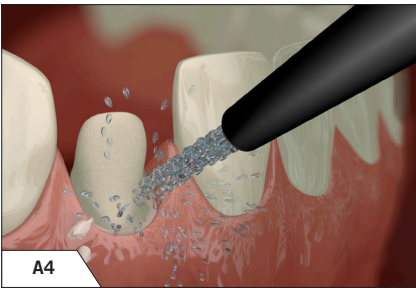














# Dental practice

**B** Preparation **B-I** metal, titanium

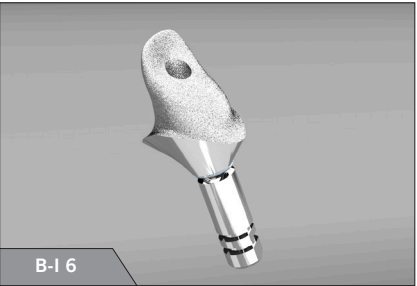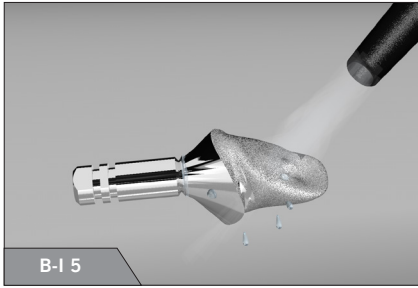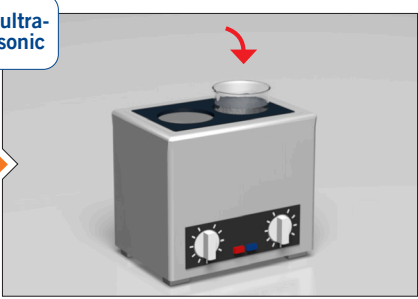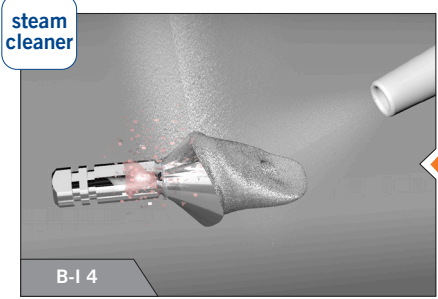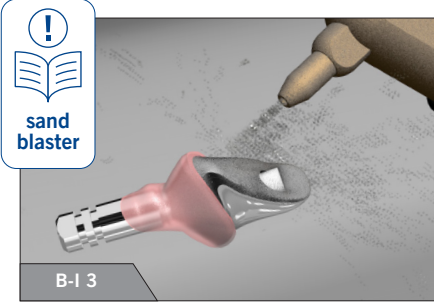







**Dental practice**

<b>B</b>	<b>Preparation</b>	<b>B-II</b>	silicate ceramic
----------	--------------------	-------------	------------------

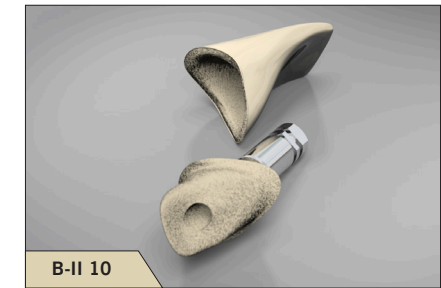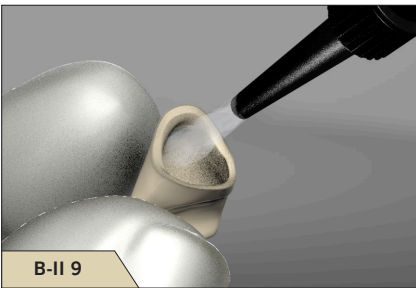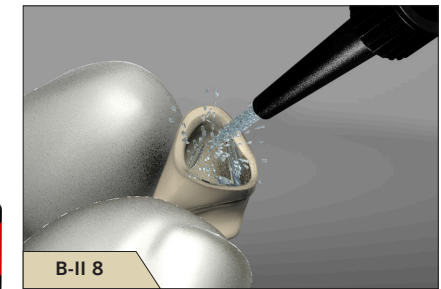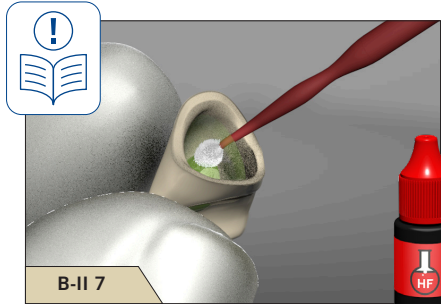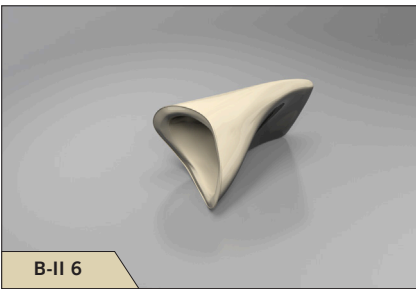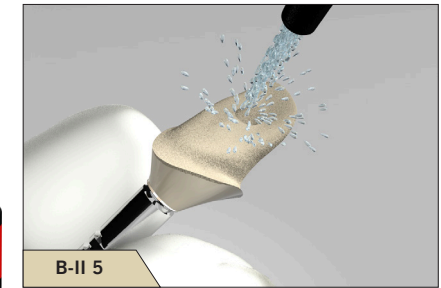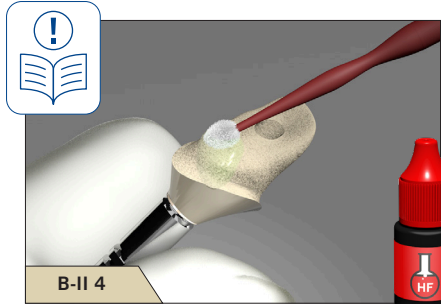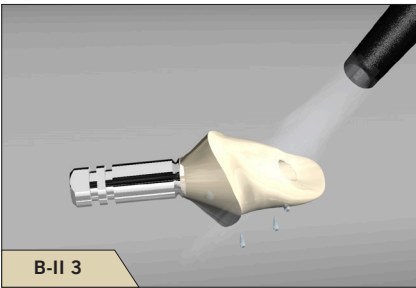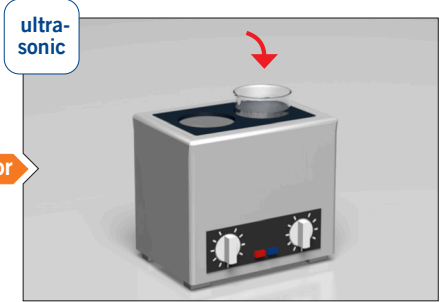
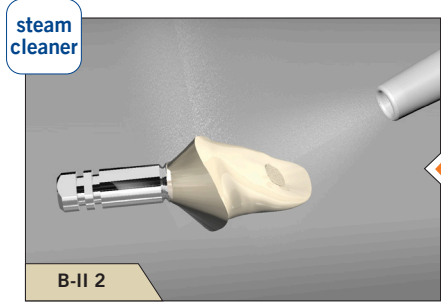
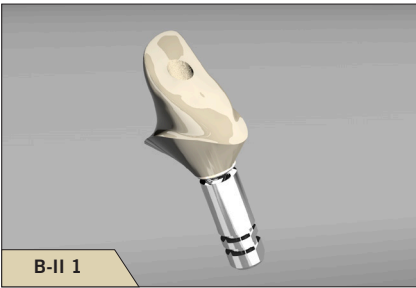


**Dental practice**


<b>B</b>	<b>Preparation</b>	<b>B-III</b>	oxide ceramic / composite
----------	--------------------	--------------	---------------------------

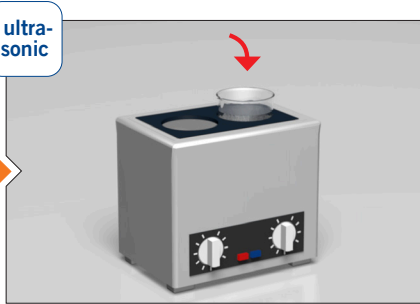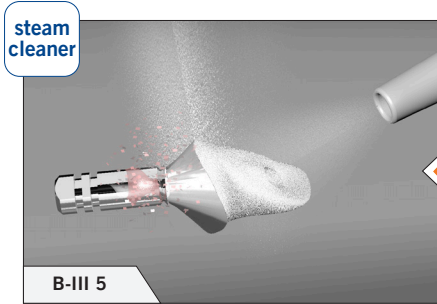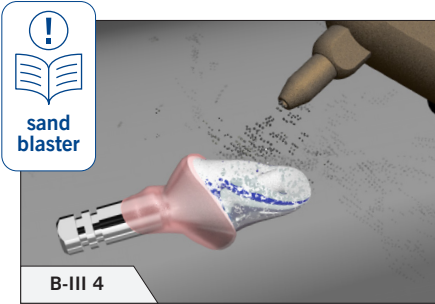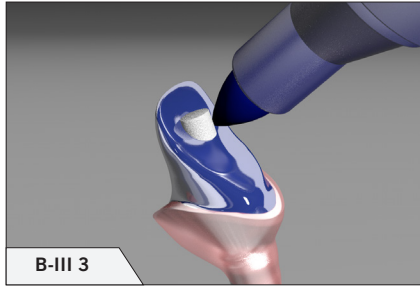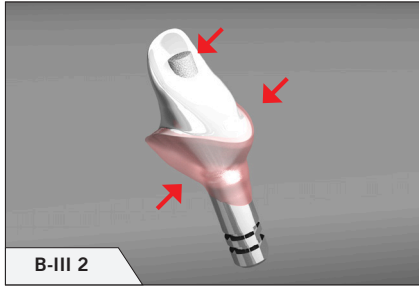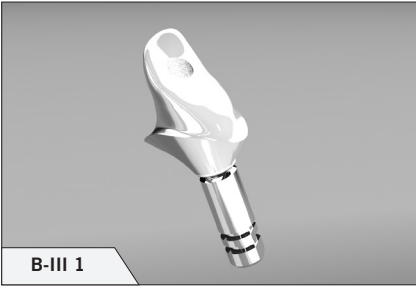

or

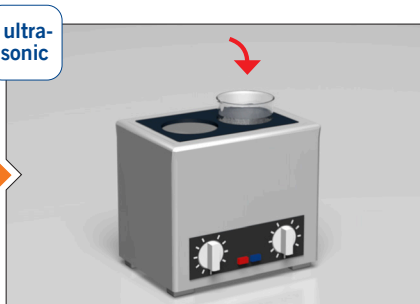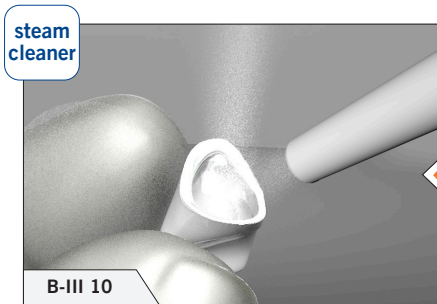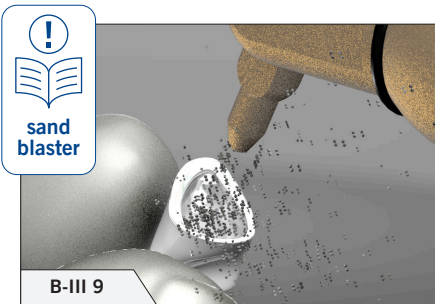

or

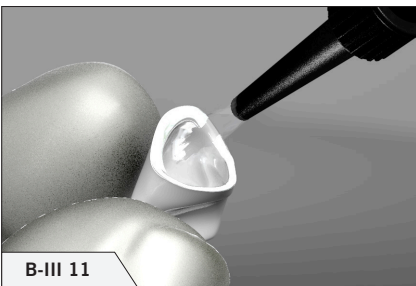

Dental practice



C Application

**C1** **C2** **C3**

**C4** **C5** **C6** **C7**

**C8** **C9** **C10**

**C11** **C12**

60 sec.

Ceramic Bond

universal

Bifix Hybrid Abutment

!

!

Glycerine

ca. 4 min.

PRESS